




# Evolution<sup>®</sup> Nitrx<sup>™</sup>

The medial-pivot knee  
shown to reduce the release  
of specific metal ions<sup>1</sup>



**MicroPort**  
Orthopedics

*Full Function, Faster<sup>®</sup>*

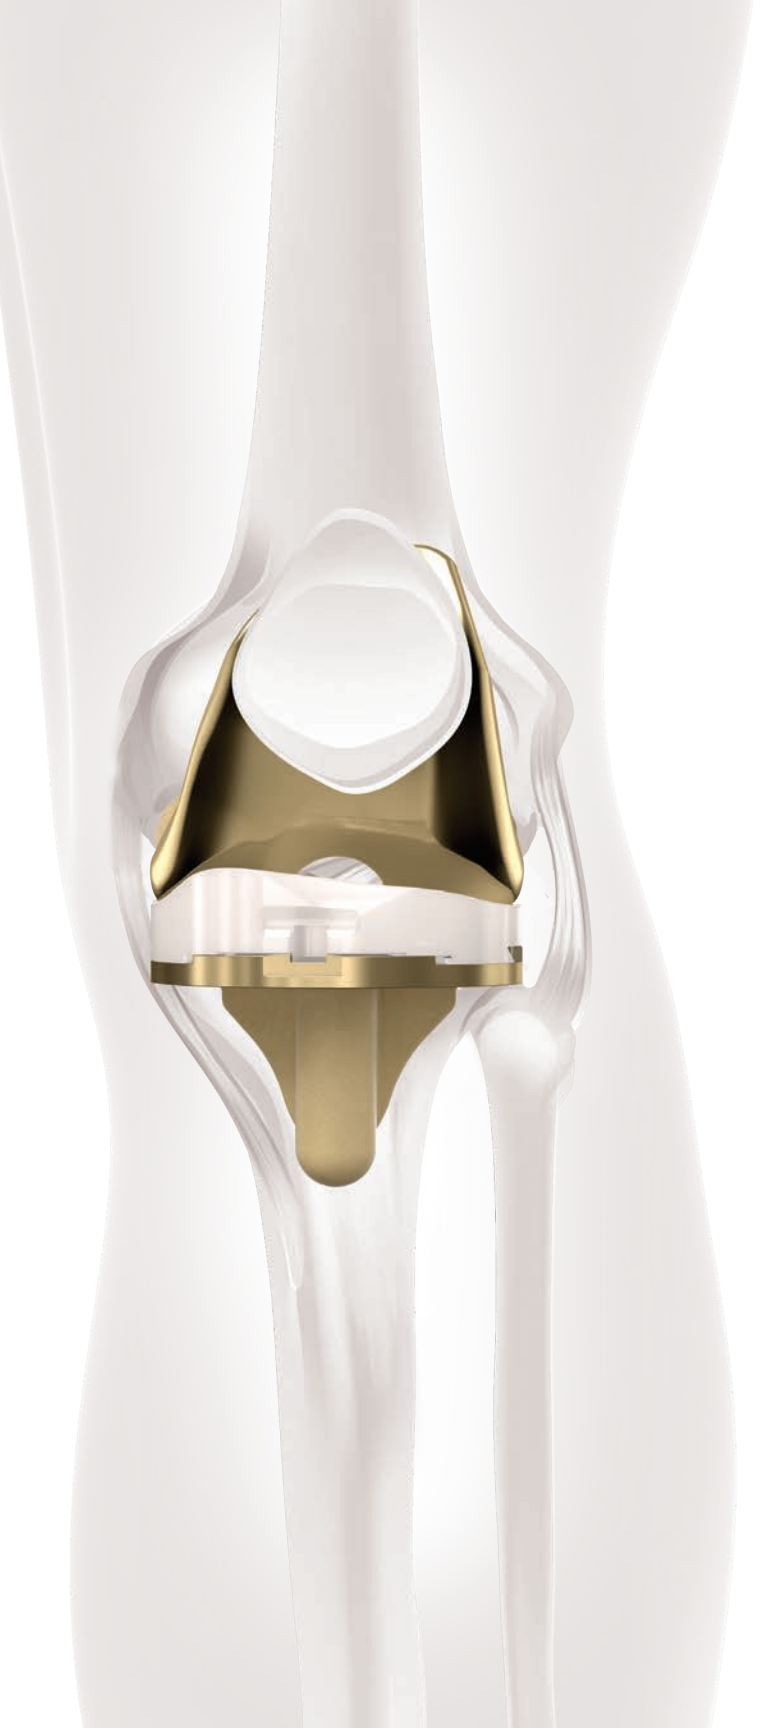

# Introduction

The MicroPort Orthopedics medial-pivot knee system now stands on over 20 years of clinically demonstrated success with its novel medial-pivot design built on the evidence of the natural stability and kinematic motion of the knee.

The Evolution® NitrX™ medial-pivot knee features a titanium niobium nitride (TiNbN) coating that has been shown to reduce the release of cobalt (Co), chromium (Cr), nickel (Ni), and molybdenum (Mb) ions common in standard CoCr implants. The Evolution® NitrX™ knee maintains the kinematic benefits of the medial-pivot design<sup>2</sup>, resulting in optimal stability.<sup>5</sup>

It has been clinically demonstrated that patients are more satisfied with the MicroPort Orthopedics medial-pivot knee design when compared to more traditional designs. This preference could be the result of the stability provided through the high tibiofemoral conformity in the medial compartment and motion provided in the lateral compartment.<sup>2</sup>


Metal sensitivity has been linked to metallic debris and metal ions, namely cobalt, chromium, and nickel. The Evolution® NitrX™ medial-pivot knee has been shown in simulated clinical testing to reduce the release of these metal ions<sup>1</sup>, and builds upon the same medial-pivot legacy of 95% patient satisfaction with 98.8% survivorship at 17 years.<sup>3</sup>

# The medial-pivot knee system


When first introduced, the medial-pivot knee proved to be a novel concept in the orthopedic community. Challenging the traditional axiom of knee kinematics, pioneers in the field, such as J. David Blaha, MD, Mr. Michael Freeman, MD, Richard Komistek, PhD, and Vera Pinskerova, PhD, provided kinematic and radiographic evidence that supported medial pivoting kinematics of the knee. This evidence demonstrated that the normal knee exhibits a fixed flexion-extension axis in the medial compartment and anterior-posterior translation in the lateral compartment during the gait cycle.

The medial-pivot knee provides a constant radius of curvature and utilizes a unique articular surface geometry to maintain medial stability throughout a greater range of motion, while allowing for the lateral condyle to move in a controlled arcuate path during flexion.


## IMAGES OF THE NORMAL KNEE<sup>5</sup>




Stable medial compartment



Mobile lateral compartment

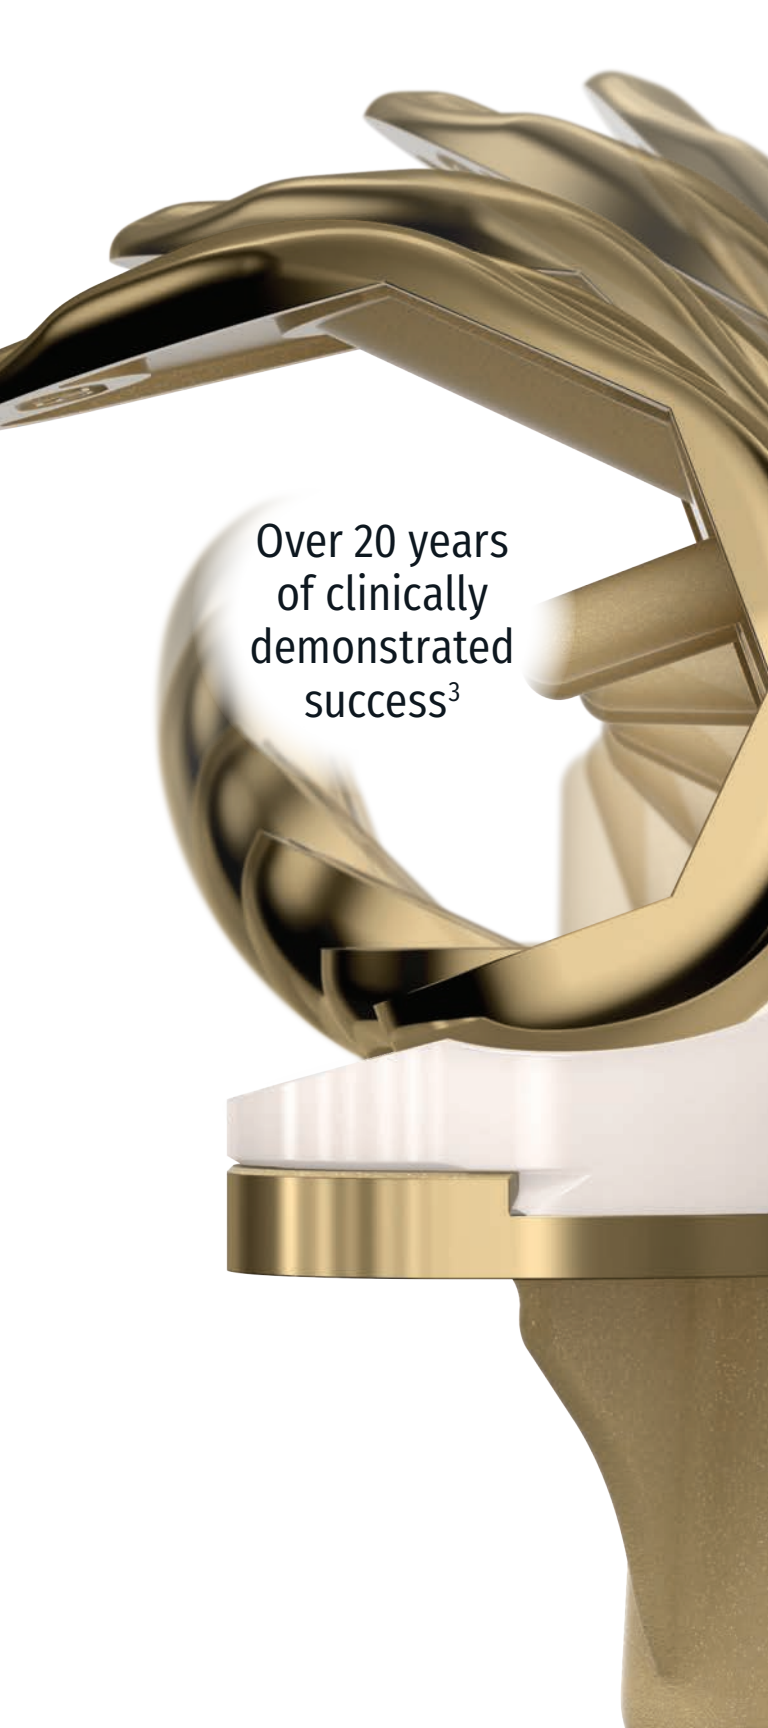A golden, stylized hand is shown holding a white pill. The hand is rendered in a metallic, reflective gold color with sharp, angular edges. The fingers are curled around the pill, which is a simple white cylinder. The background is plain white, making the golden hand and the pill stand out prominently.

Over 20 years  
of clinically  
demonstrated  
success<sup>3</sup>

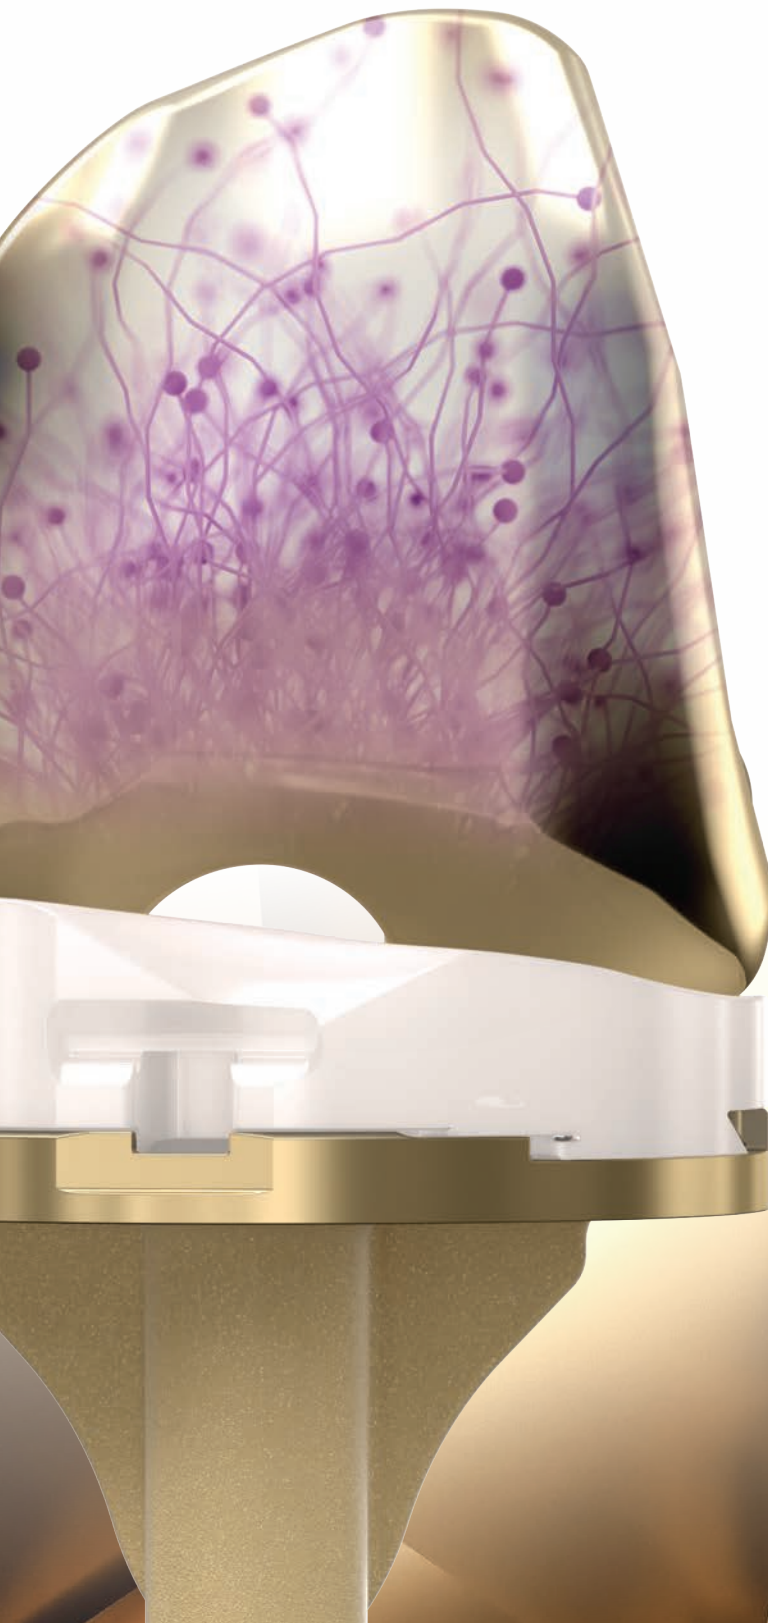

# Reduce the release of specific metal ions while promoting natural kinematics<sup>1,2</sup>

The Evolution® NitrX™ knee features a titanium niobium nitride (TiNbN) coating, which creates a barrier against the potential release of metal ions common in cobalt chrome (CoCr) implants.<sup>1</sup> Since metal sensitivity in patients is linked to metallic debris and metal ions, namely cobalt, chromium and nickel, preventing that debris from interacting with soft tissue may have a benefit of reducing the incidence of tissue reactions.<sup>6,7</sup>



## Excellent wear properties<sup>4</sup>

Long term wear is one reason for revision in the long term. The Evolution® NitrX™ titanium niobium nitride (TiNbN) coating demonstrated the same excellent wear characteristics as a CoCr prosthesis.<sup>1</sup>

## Hardness of different types of surface treatments in GPa

TiNbN **24.5**<sup>4</sup>

Oxinium **12.1**<sup>15</sup>

CoCr **3**<sup>15</sup>





**Excellent  
biocompatibility<sup>1,4</sup>**



**High corrosion  
resistance<sup>8-11</sup>**



**Increased hardness  
and wettability<sup>1,4</sup>**

Evolution® NitrX™'s TiNbN coating is 4 to 5 times harder than conventional CoCr<sup>4,15</sup> and is twice as hard as Smith and Nephew's OXINIUM™.<sup>4,15</sup>



# Patients feel the difference

Patients in a peer-reviewed study that examined patient satisfaction among patients who underwent bilateral staged total knee replacement with different prostheses preferred the MicroPort Orthopedics medial-pivot design equally to an ACL/PCL retaining prosthesis and more than all other designs (CR, PS, and Mobile-Bearing).<sup>12</sup>

# Focus on rapid recovery

Surgeons utilizing the medial-pivot knee system have stated that their patients recover faster and are back to activities of daily life sooner than traditional knee replacements.<sup>13</sup>

## IMPROVED STABILITY

Designed with a single radius in all planes, and a medial “socket” on the insert, the Evolution® medial-pivot knee system provides stability throughout all phases of flexion. Additionally, the medial anterior lip acts to replace the PCL and minimize anterior femoral sliding while the posterior lip replaces the ACL in an effort to stop posterior slide.

## PROMOTES NATURAL KINEMATICS

The unique design of the Evolution® tibial insert substitutes for both the ACL and PCL, as well as the natural contours of the knee to promote normal kinematics.<sup>16</sup>

## EXCELLENT OUTCOMES

The Evolution® medial-pivot knee system is built upon a legacy of 95% patient satisfaction with 98.8% survivorship at 17 years<sup>3</sup>, and features a design that enhances quadriceps efficiency, allowing for improved proprioception.<sup>16</sup>



The CE-Marking of Conformity is applied per catalog number and appears on the outer package label, if applicable.

Trademarks and Registered marks of MicroPort Orthopedics Inc. OXINIUM™ is a registered trademark of Smith and Nephew



MicroPort Orthopedics Inc.  
5677 Airline Road  
Arlington, TN USA 38002  
866 872 0211

microportortho.com

© 2019 MicroPort Orthopedics Inc. All Rights Reserved. 017884 MAY2019

#### References

- <sup>1</sup> MPO Data on file
- <sup>2</sup> Dennis DA, Komistek RD, Mahfouz MR, Haas BD, Stiehl JB. Multicenter determination of in vivo kinematics after total knee arthroplasty. *Clin Orthop Relat Res.* 2003
- <sup>3</sup> Macheras GA et al A long term clinical outcome of the Medial Pivot Knee Arthroplasty System. *Knee.* 2017 Mar;24(2):447-453
- <sup>4</sup> [http://dot-coatingsusa.com/images/pdf/protection\\_against\\_allergic\\_reactions\\_through\\_ceramic\\_coatings.pdf](http://dot-coatingsusa.com/images/pdf/protection_against_allergic_reactions_through_ceramic_coatings.pdf)
- <sup>5</sup> Freeman MA, Pinskerova V. The movement of the knee studied by magnetic resonance imaging. *Clin Orthop Relat Res.* 2003;410:35-43
- <sup>6</sup> Lachiewicz, Watters, Jacobs. "Metal Hypersensitivity and Total Knee Arthroplasty." *J Am Acad Orthop Surg.* 2016 February ; 24(2): 106-112. doi:10.5435/JAAOS-D-14-00290
- <sup>7</sup> Hallab, Merrit, Jacobs. "Metal Sensitivity in Patients with Orthopaedic Implants." *J. Bone Joint Surg. Am.* 83:428-, 2001.
- <sup>8</sup> Kirmanidou, Yvoni et al. "New Ti-Alloys and Surface Modifications to Improve the Mechanical Properties and the Biological Response to Orthopedic and Dental Implants: A Review." *BioMed Research International* 2016 (2016): 2908570. PMC. Web. 1 Oct. 2018
- <sup>9</sup> R. Thull, Corrosion behavior of dental alloys coated with Titanium Niobium Oxinitride, *Deutsche Zahnärztliche Zeitschrift* 1991Nov., Universität Würzburg
- <sup>10</sup> Test report DOT GmbH and Nordum GmbH, Examination of influence of PVD – coatings to the ion release of CoCrMo-alloys in SBF – buffer, 2006
- <sup>11</sup> Hayashi Y., Nakayama G. Corrosion behavior in subcritical and supercritical water containing sodium chloride. *Corrosion Engineering, Science and Technology.* 2002;31(6):491-494.
- <sup>12</sup> Pritchett JW. Patients prefer a bicruciate-retaining or the medial pivot total knee prosthesis. *J Arthroplasty.* 2011;26(2):224-8
- <sup>13</sup> Cassard et al, Outpatient TKR – 30 days readmission rate and complications, Full Function Faster meeting, London, 2018.
- <sup>14</sup> CermTec AG. BILOX delta nanocomposite for arthroplasty The fourth generation of Ceramics: Scientific information and performance data
- <sup>15</sup> M. Long, L. Riester, and G. Hunter, "Nano-hardness measurements of oxidized Zr-2.5Nb and various orthopaedic materials", *Trans. Soc. Biomaterials*, 21, 1998, p. 528.
- <sup>16</sup> Lamontagne, M.; Czornyj, C; Dervin, G. Functional performance and muscle activation with an ACL-PCL substituting knee. Podium Presentation, ACBS 2012.